Calibration of Hydrostatic Pressure Tester (Pressure and Temperature)

Description




Hydrostatic Pressure Tester

- Download driver


AHP PLASTIK MAKINA

DTCOM Download


- Click on DTCOM_E.exe

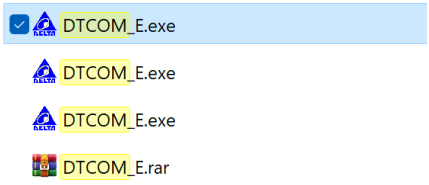

- Select COM port (Refer to COM port driver installation guide) and then click on â€œAuto Detectâ€•.

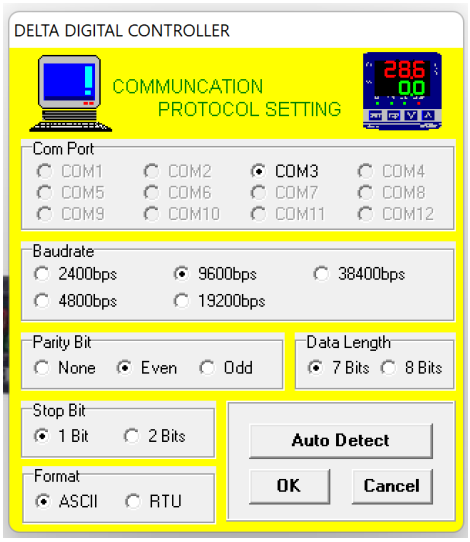

- After detection of some controllers, in the â€œcommunication protolâ€• section click on one the detected items and then click â€œSETâ€• then â€œCloseâ€•.








- Click on Monitor Icon.




AHP PLASTIK MAKINA


- Select proper â€œAddressâ€•. In hydrostatic pressure testers from AHP, there are â€œnumber of lines+1â€• station address, for example in 4 station hydrostatic unit there are 5 address. 1 to 4 is related to pressure lines and 5 is related to temperature address. Select requested address for calibration.

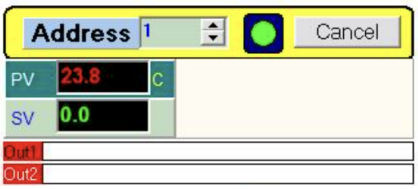



- In the bottom of page settings for the requested station address will be shown.

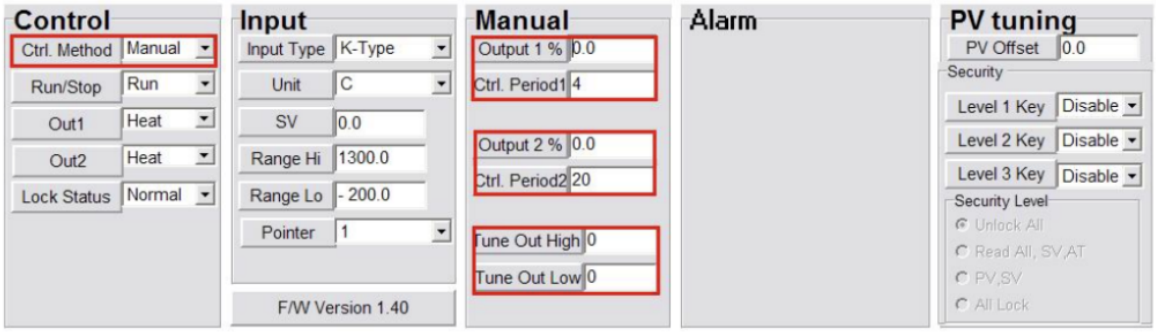

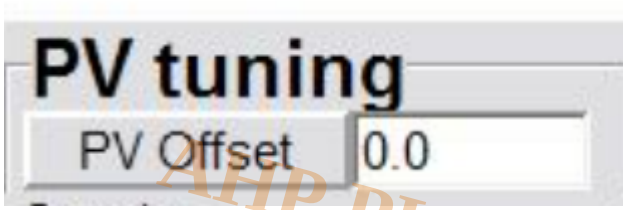

AHP PLASTIK MAKINA

Calibration offset value. Be noted after set of proper value donâ€™t forget to â€œENTERâ€•.

- Donâ€™t change any other parameters of this page.
- You can do same procedure for temperature line as well.

Category

1. Software Guide